

**ROTANODE™  
E7239X  
E7239FX  
E7239GX**

**Rotating Anode X-ray Tube Assembly**

- ◆ Rotating anode X-ray tube assembly for the purpose of general diagnostic X-ray procedures.
- ◆ Specially processed Rhenium-tungsten faced molybdenum target of 74 mm diameter.
- ◆ These tubes have foci 2.0 and 1.0, and are available for a maximum tube voltage 125 kV.
- ◆ Accommodated with IEC60526 type high-voltage cable receptacles.



**General Data**

**IEC Classification (IEC60601-1:2005+A1:2012) ..... Class I ME EQUIPMENT**

**Electrical:**

Circuit:

High Voltage Generator ..... Constant Potential High-Voltage Generator  
 Grounding ..... Center-grounded

Nominal X-ray Tube Voltage:

Radiographic ..... 125 kV

Nominal Focal Spot Value:

Large Focus ..... 2.0  
 Small Focus ..... 1.0

Nominal Anode Input Power (at 0.1s):

	60 Hz	50 Hz
Large Focus .....	47 kW	42.5 kW
Small Focus .....	22.5 kW	21 kW

Nominal Radiographic Anode Input Power:

	60 Hz	50 Hz
Large Focus .....	47 kW	42.5 kW
Small Focus .....	22.5 kW	21 kW

★The information contained herein is presented only as a guide for the application of our products. No responsibility is assumed by Canon Electron Tubes & Devices Co., Ltd. (CETD) for any infringements of patents or other rights of the third parties which may result from its use. No license is granted by implication or otherwise under any patent or patent rights of CETD or others.  
 ★The information contained herein may be changed without prior notice. It is therefore, advisable to contact to CETD before processing with the design of equipment incorporating this product.

## Motor Ratings:

Stator: XS-AV

		Starting		Running
		50/60		50/60
Driven Frequency	[Hz]	50/60		50/60
Input Power	[W]	1050	270	43
Voltage <sup>1) 3)</sup>	[V]	200	100	40
Current <sup>2)</sup>	[A]	6.0	3.0	1.2
Min. Speed Up <sup>4)</sup>	[s]	0.8	1.5	-
Capacitor	[ $\mu$ F]	24	24	24

Note: 1) Applied voltage between common and main terminal.

2) Common current.

3) The every applied voltage must be never exceeded 110% of the above specification.

4) The speed-up time is allowed up to 110% of the above specification.

## Anode Speed:

60 Hz ..... Minimum 3200 min<sup>-1</sup>50 Hz ..... Minimum 2700 min<sup>-1</sup>

## Stator Resistance:

Common-Main Winding ..... 27.5  $\Omega$ Common-Auxiliary Winding ..... 58.0  $\Omega$ Resistance Between Housing and Low Voltage Terminals ..... Minimum 2 M $\Omega$ 

Normal Operating Range of the Housing Temperature ..... 16 ~ 75 °C

Mode of Operation ..... Intermittent

**Mechanical:**

Dimensions ..... See dimensional outline

Overall Length ..... 479 mm

Maximum Diameter ..... 152.4 mm

## Target:

Anode Angle ..... 16 degrees

Diameter ..... 74 mm

Construction ..... Rhenium-Tungsten faced Molybdenum

## Filtration:

Permanent Filtration ..... 0.9 mm Al / 75 kV IEC60522:1999

Available Additional Filter combination (0.4 - 1.5 mm) ..... Maximum 2.4 mm Al / 75 kV

## Radiation Protection (In accordance with IEC60601-1-3:2008):

Leakage Technique Factor ..... 125 kV, 4 mA

X-ray Coverage ..... 354 × 354 mm at SID 750 mm

Weight (Approx.) ..... 16 kg

High Voltage Receptacle ..... To meet the requirements of IEC60526 Corrigendum1:2010

Cooling Method ..... Natural or forced air

## Tube Housing Model Number:

E7239X ..... XH-121

E7239FX ..... XH-126

E7239GX ..... XH-150

## Absolute Maximum and Minimum Ratings

(At any time, these values must not be exceeded.)

### Maximum X-ray Tube Voltage:

Radiographic .....	125 kV
Between Anode (or Cathode) and Ground .....	62.5 kV

Minimum X-ray Tube Voltage ..... 40 kV

Maximum X-ray Tube Current: ..... See rating charts

    Large Focus .....

    Small Focus .....

### Maximum Filament Current:

    Large Focus .....

    Small Focus .....

### Filament Voltage:

    Large Focus (At maximum filament current 5.1 A) .....

    Small Focus (At maximum filament current 5.1 A) .....

Filament Frequency Limits ..... 0 ~ 25 kHz

Continuous Anode Input Power ..... 60 W (85HU/s)

### Thermal Characteristics:

    Anode Heat Content .....

    Maximum Anode Heat Dissipation .....

    X-ray Tube Assembly Heat Content .....

### Nominal Continuous Input Power:

    Without Air-circulator .....

## Environmental Limits

### Operating Limits:

    Temperature .....

    Humidity .....

(No condensation)

    Atmospheric Pressure .....

### Shipping and Storage Limits:

    Temperature .....

    Humidity .....


(No condensation)

    Atmospheric Pressure .....


## Maximum Rating Charts (Absolute Maximum Rating Charts)

Conditions: Tube Voltage  
Constant Potential High-Voltage Generator  
Stator Power Frequency 60Hz

Nominal Focal Spot Value: 2.0 ■

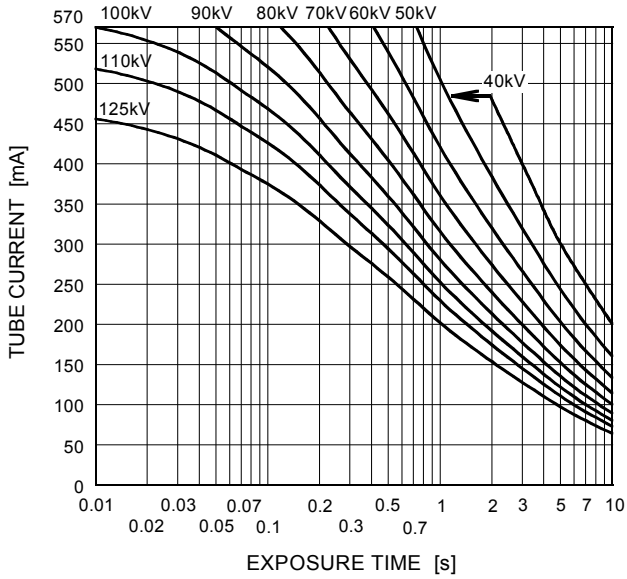


Nominal Focal Spot Value: 1.0 □

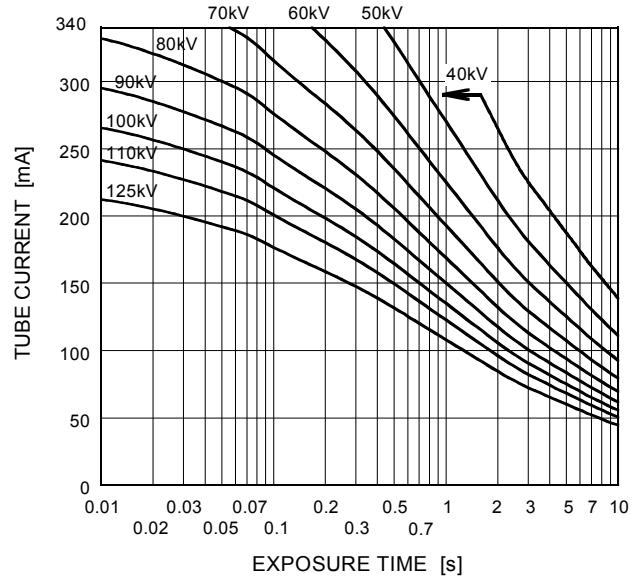


Conditions: Tube Voltage  
Constant Potential High-Voltage Generator  
Stator Power Frequency 50Hz

Nominal Focal Spot Value: 2.0 ■

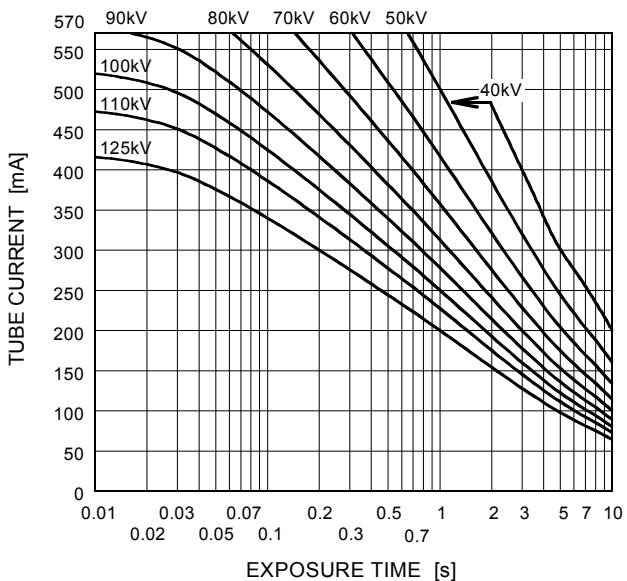


Nominal Focal Spot Value: 1.0 □

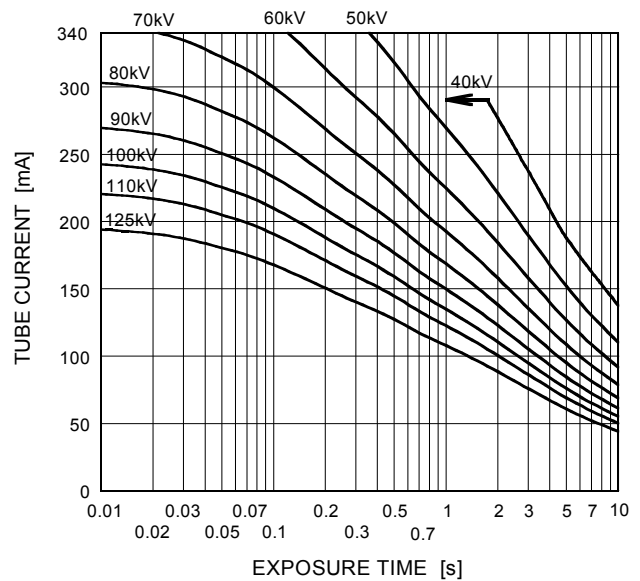

## Emission & Filament Characteristics


Constant Potential High-Voltage Generator

Nominal Focal Spot Value: 2.0 ■

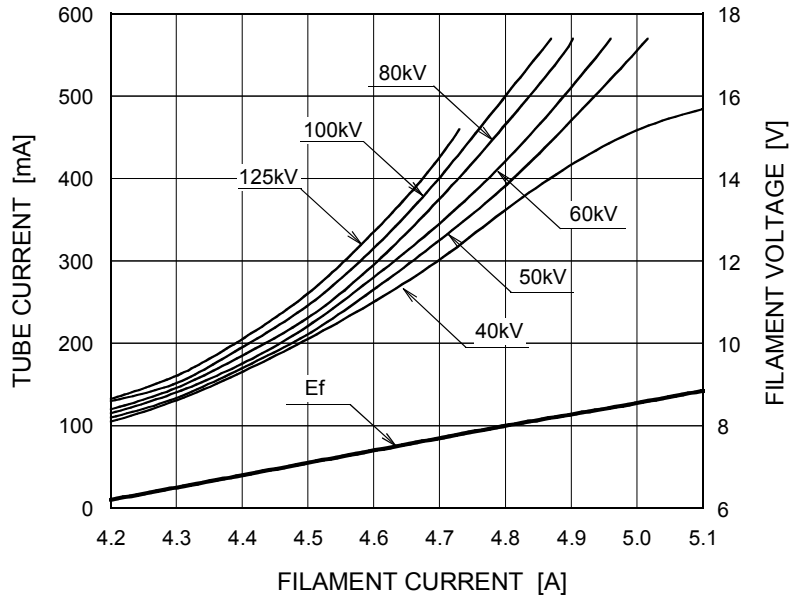

For Reference Only


Nominal Focal Spot Value: 1.0 □

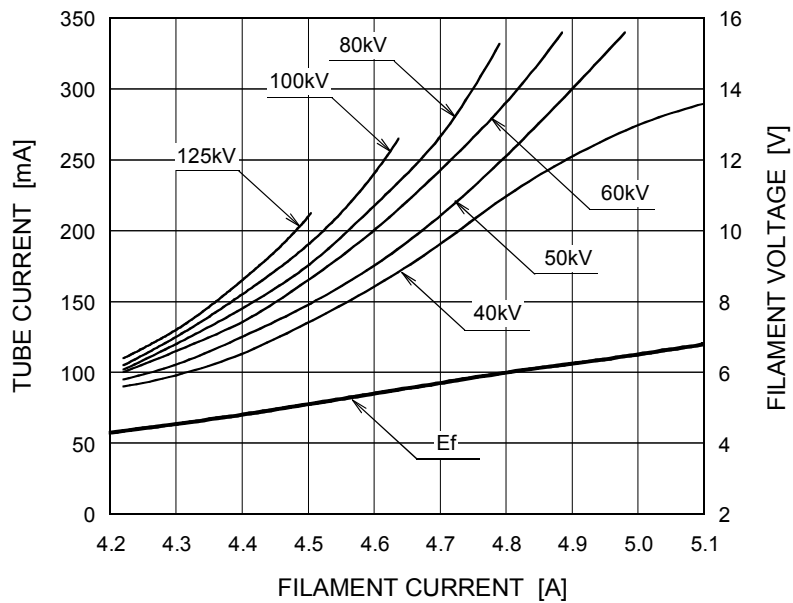


For Reference Only

## Thermal Characteristics

X-ray Tube Assembly Heating / Cooling Curve

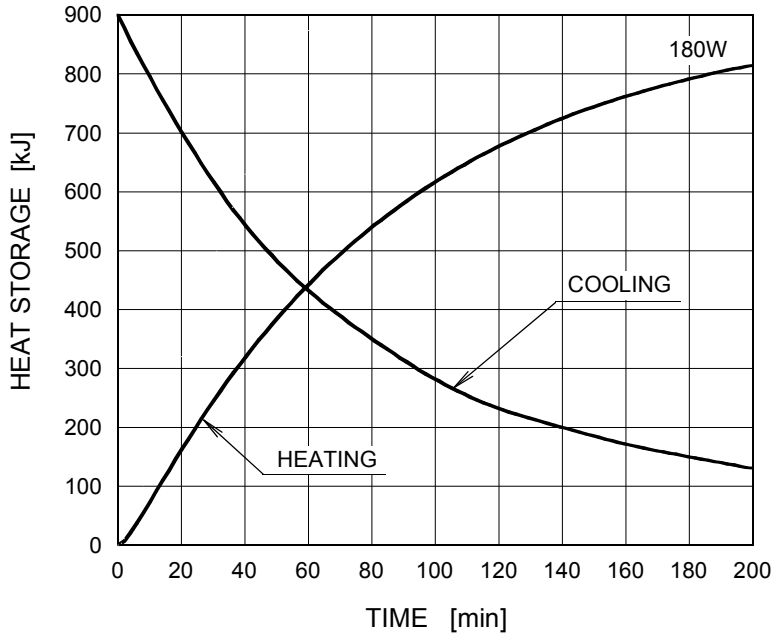




Anode Heating / Cooling Curve

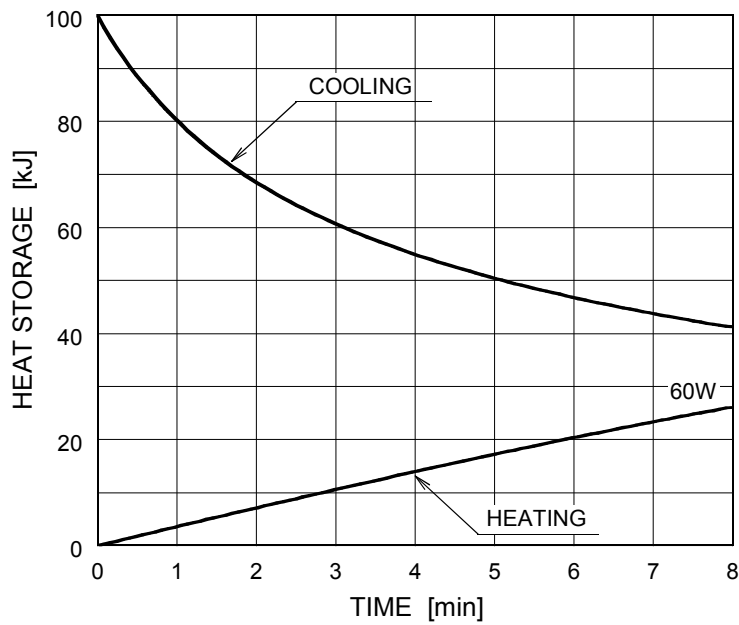

The heating curves are showing example of average input power to anode in operation.

### Dimensional Outline of E7239X

Unit mm

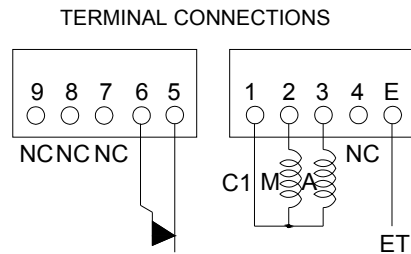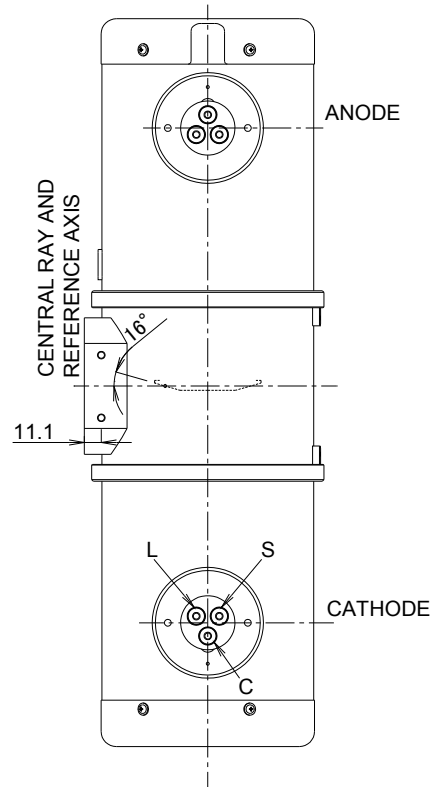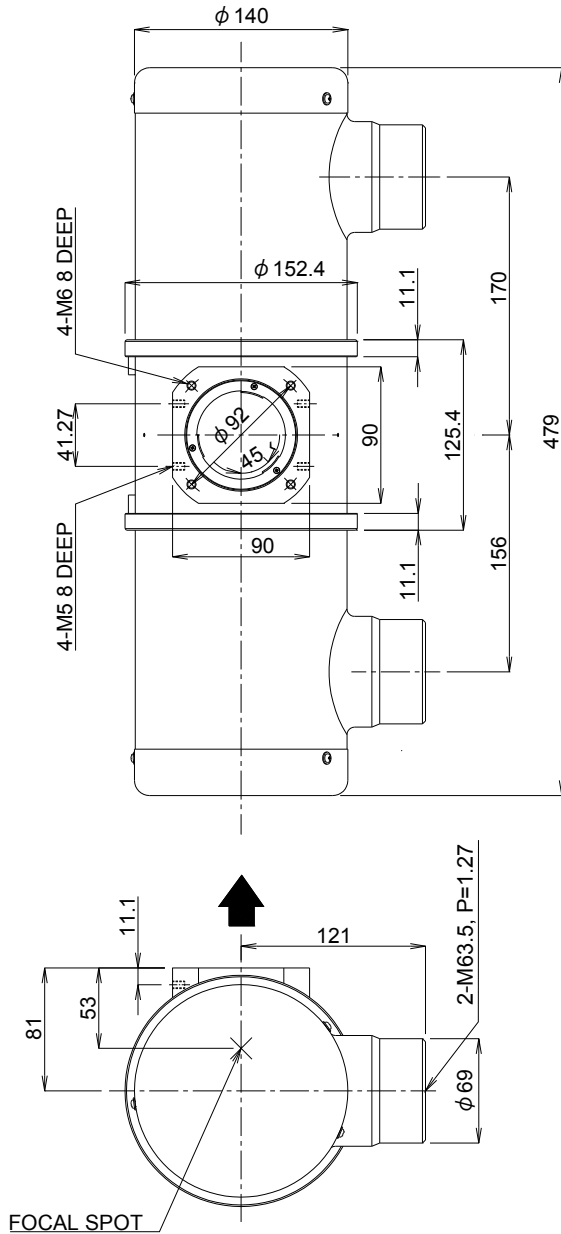


TEMPERATURE RELAY (NORMALLY CLOSED)

Note) Do not connect terminal No.1 and No.5 or 6 in series circuit.

**CATHODE TERMINAL**  
 C : COMMON  
 L : LARGE FOCUS  
 S : SMALL FOCUS

**TERMINAL CONNECTIONS**  
 C1 : COMMON  
 M : MAIN WINDING OF THE STATOR  
 A : AUX. WINDING OF THE STATOR  
 NC : NON-CONNECTION  
 ET : EARTH TERMINAL


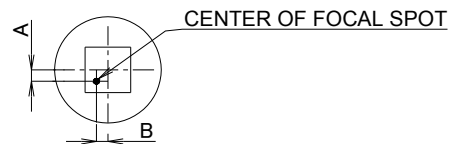


$-1.5\text{mm} \leq A \leq 1.5\text{mm}$   
 $-1.5\text{mm} \leq B \leq 1.5\text{mm}$

▲ : CENTRAL X-RAY ANODE & CATHODE TERMINAL : IEC60526 TYPE


### Dimensional Outline of E7239FX

Unit mm

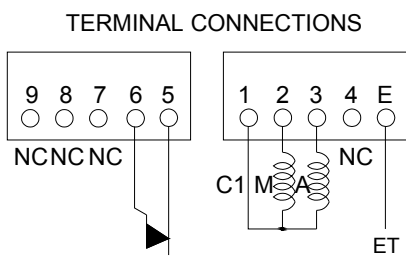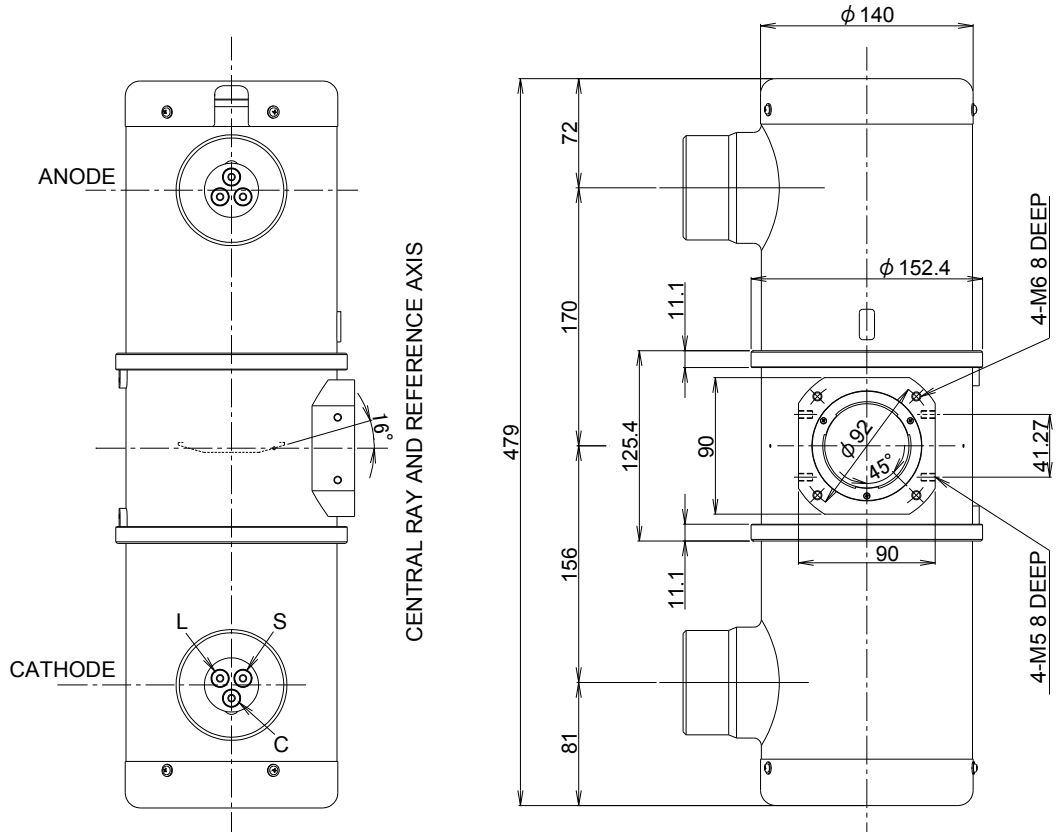


TEMPERATURE RELAY (NORMALLY CLOSED)

Note) Do not connect terminal No.1 and No.5 or 6 in series circuit.

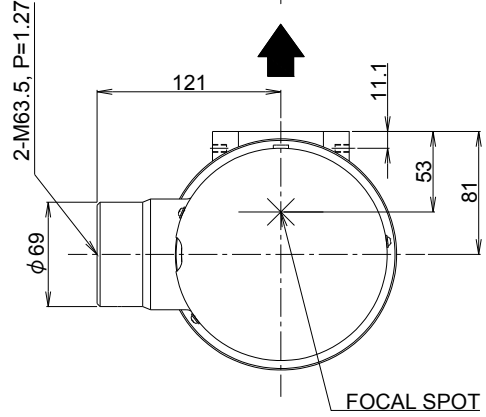

CATHODE TERMINAL  
 C : COMMON  
 L : LARGE FOCUS  
 S : SMALL FOCUS

TERMINAL CONNECTIONS  
 C1 : COMMON  
 M : MAIN WINDING OF THE STATOR  
 A : AUX. WINDING OF THE STATOR  
 NC : NON-CONNECTION  
 ET : EARTH TERMINAL

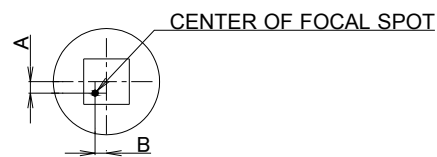


-1.5mm ≤ A ≤ 1.5mm  
 -1.5mm ≤ B ≤ 1.5mm

▲ : CENTRAL X-RAY ANODE & CATHODE TERMINAL : IEC60526 TYPE



## Dimensional Outline of E7239GX

Unit mm

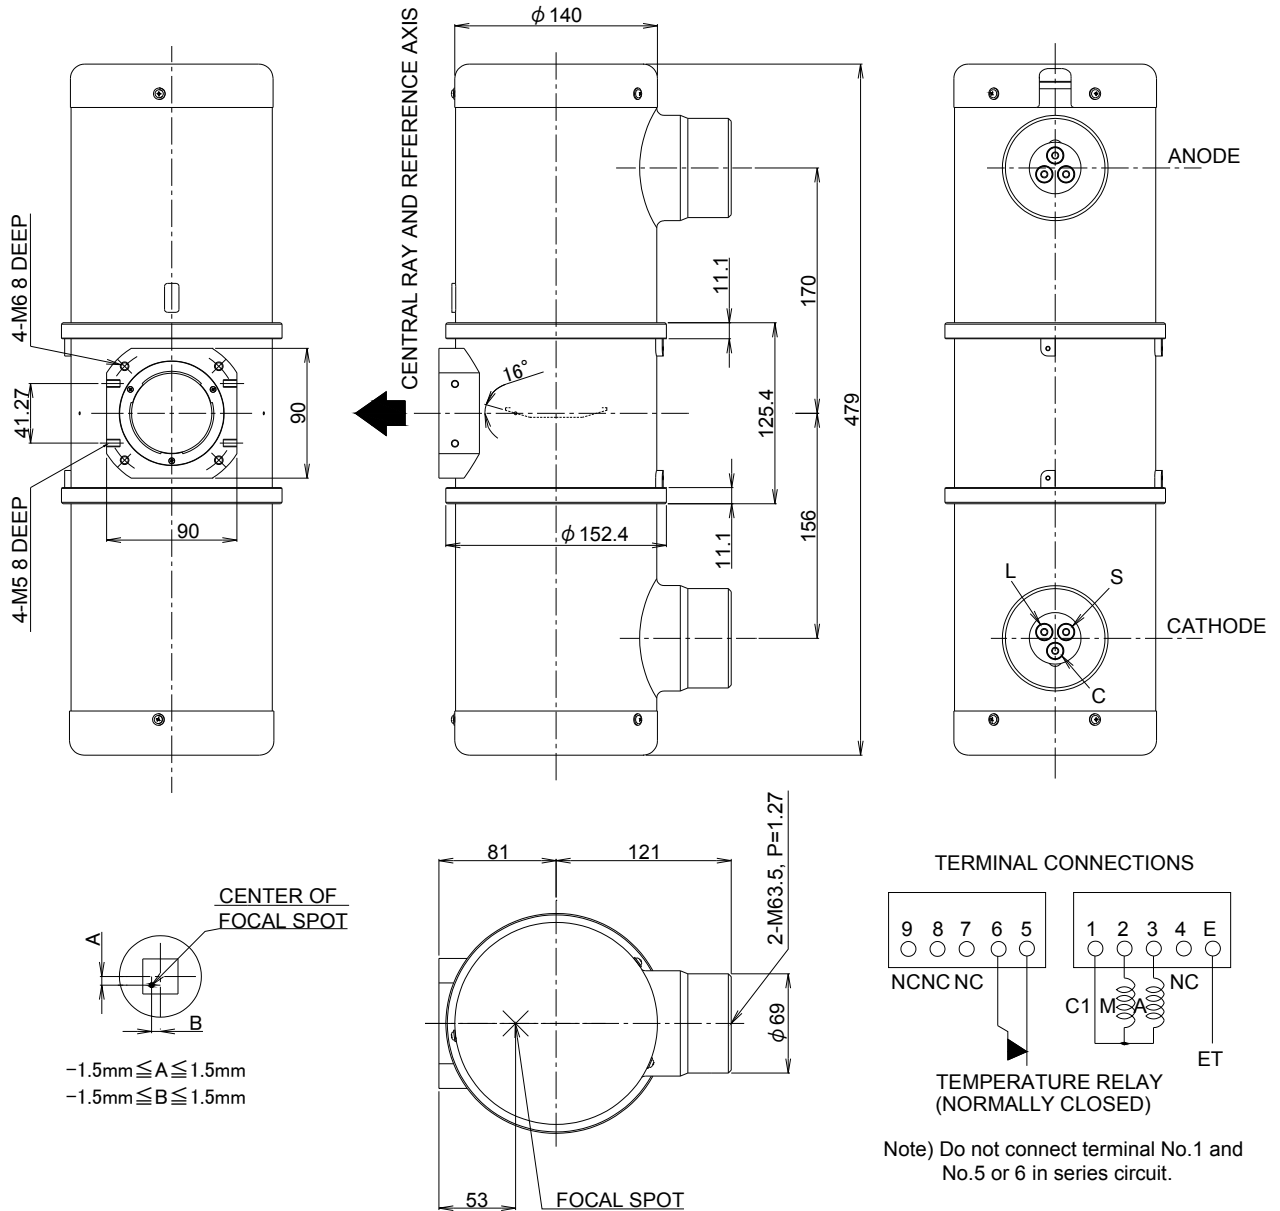

### EXPLANATION OF SYMBOLS

#### CATHODE TERMINAL


- C : COMMON
- L : LARGE FOCUS
- S : SMALL FOCUS

#### TERMINAL CONNECTIONS

- C1 : COMMON
- M : MAIN WINDING OF THE STATOR
- A : AUX. WINDING OF THE STATOR
- NC : NON-CONNECTION
- ET : EARTH TERMINAL

- ▲ : CENTRAL X-RAY ANODE & CATHODE TERMINAL
- : IEC60526 TYPE

---

 **CANON ELECTRON TUBES & DEVICES CO., LTD.**  
Marketing Engineering Group, Sales Department  
1385, Shimoishigami, Otawara-shi, Tochigi 324-8550, Japan  
Tel: +81-287-26-6666 Fax: +81-287-26-6060  
<https://etd.canon>

·The head office of Canon Electron Tubes & Devices Co., Ltd. has been certified to meet all the requirements of Environmental Management System ISO14001.  
·Canon Electron Tubes & Devices Co., Ltd. has been certified to meet all the requirements of Quality Management Systems ISO9001 and ISO13485.  
Product scope is referred to the following URL. <https://etd.canon/eng/company/quality.htm>.